

INTERNATIONAL CALIBRATION ORDER FORM


© 2017 STANDARD IMAGING, INC. 4836-00, 10/17 PAGE 1 OF 2

Standard Imaging offers calibrations from the Accredited Dosimetry Calibration Laboratory (ADCL). Only one purchase order is needed to cover calibrations, shipping/handling and service. All Standard Imaging instruments are tested and examined prior to calibration. If service is required, we'll call you for your approval prior to the repair.

To *expedite your order*, simply:

1. Print and fill out the Calibration Order Form, and
2. Send your equipment, purchase order and Calibration Order Form to Standard Imaging.
3. If service is needed, please authorize a dollar amount we can charge without checking back with you to ensure a faster response. We'll take care of the rest of the process for you!

NOTE: Prices are subject to change without notice.

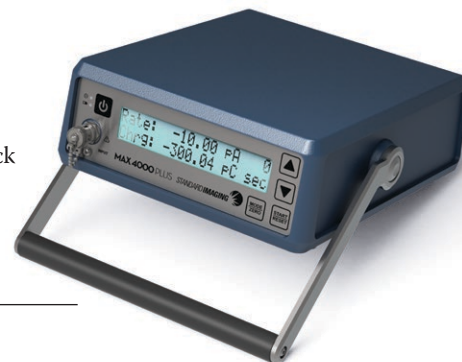

ELECTROMETER CALIBRATION

(All Makes and Models)

Initial set-up and 1 scale calibration is \$ ____.

Each additional calibrated scale is \$ ____ each.

| | | | |
|--------------------------|----------|--|-------------------------------|
| <input type="checkbox"/> | 80015-1 | Initial set-up and 1 scale calibration | \$ |
| <input type="checkbox"/> | 80015-2 | Initial set-up and 2 scale calibrations for CDX 2000, 2000A, 2000B or Premier 3000 | \$ |
| <input type="checkbox"/> | 80015-4 | Initial set-up and four scale calibrations for MAX 4000 | \$ |
| <input type="checkbox"/> | 80015-8 | Initial set-up and eight scale calibrations for SuperMAX | \$ |
| <input type="checkbox"/> | 80015-16 | Initial set-up and sixteen scale calibrations for the TomoElectrometer | \$ |
| | | Number of additional scale calibrations at \$ ____ each | Quantity <input type="text"/> |

EXTERNAL BEAM THERAPY ION CHAMBER CALIBRATION

(All Makes and Models)

Initial set-up and one cobalt calibration point in air or water is \$ ____.

Each additional calibration point for the same chamber is \$ ____.

| | | | |
|--------------------------|---------|--|----|
| <input type="checkbox"/> | 80031 | Therapy Ionization Chamber Calibration, Cobalt point in WATER, 1 st point | \$ |
| <input type="checkbox"/> | 80031-2 | Therapy Ionization Chamber Calibration, Cobalt point in WATER, 2 nd point | \$ |
| <input type="checkbox"/> | 80032 | Therapy Ionization Chamber Calibration, Cobalt point in AIR, 1 st point | \$ |
| <input type="checkbox"/> | 80032-2 | Therapy Ionization Chamber Calibration, Cobalt point in AIR, 2 nd point | \$ |
| <input type="checkbox"/> | 80033 | Therapy Ionization Chamber Calibration, Cesium point, 1 st point | \$ |
| <input type="checkbox"/> | 80033-2 | Therapy Ionization Chamber Calibration, Cesium point, 2 nd point | \$ |
| <input type="checkbox"/> | 80013 | Survey Meter Calibration | \$ |

WELL CHAMBER CALIBRATION

When returning your well chamber for calibration, include your source holders for the sources to be calibrated. Your specific source holders must be used by the ADCL for the calibrations.

HDR IRIIDIUM: Initial set-up and calibration for HDR Iridium in the HDR 1000 Plus or the IVB 1000 is \$ ____.

Each additional LDR source calibration is \$ ____.

LDR SOURCES: Initial set up and calibration of one LDR source in the HDR 1000 Plus or the IVB 1000 is \$ ____.

Each additional LDR source calibration is \$ ____.



HDR IRIIDIUM WELL CHAMBER CALIBRATIONS

| | | | |
|--------------------------|-------|--|----|
| <input type="checkbox"/> | 80010 | Calibration for HDR Ir-192 in either HDR 1000 Plus or IVB 1000 | \$ |
|--------------------------|-------|--|----|

continued on back side >

INTERNATIONAL CALIBRATION ORDER FORM

© 2017 STANDARD IMAGING, INC. 4836-00, 10/17 PAGE 2 OF 2

LDR BRACHY THERAPY CALIBRATIONS AVAILABLE FOR THE HDR 1000 PLUS & THE IVB 1000

| | | |
|---------|--|----|
| 80020 | Calibration for Cesium 137 | \$ |
| 80020-B | Calibration for Cesium C-131 | \$ |
| 80025-B | Calibration for Low Dose Rate Ir-192, Best Medical International | \$ |
| 80040-D | Calibration for Iodine, Best Medical International | \$ |
| 80040-E | Calibration for Iodine, Theragenics (AGX 100) | \$ |
| 80040-K | Calibration for Iodine, Source Tech/Bard | \$ |
| 80040-M | Calibration for Iodine, SelectSeed I-125/Nucletron - Isotron | \$ |
| 80040-O | Calibration for Iodine, IsoAid Advantage-I125 | \$ |
| 80040-R | Calibration for Iodine, Eckert & Ziegler BEBIG I25.S17 | \$ |
| 80040-S | Calibration for Iodine, Eckert & Ziegler BEBIG I25.S06 | \$ |
| 80035-B | Calibration for Palladium, Theragenics | \$ |
| 80035-C | Calibration for Palladium, Best Medical International | \$ |
| 80035-E | Calibration for Palladium IsoAid Advantage-PD-103 | \$ |

INTRAVASCULAR BRACHY THERAPY CALIBRATIONS AVAILABLE FOR THE IVB 1000 ONLY

| | | |
|-----------|--|----|
| 80036-3.5 | Calibration for Sr90/Y90, 3.5 French Catheter Novoste in Source Holder 70036 | \$ |
|-----------|--|----|

SOURCE HOLDERS FOR HDR 1000 PLUS CHECK ONLY IF YOU WANT TO PURCHASE A NEW SOURCE HOLDER

| | | |
|-------|--|----|
| 70010 | Source Holder for HDR Iridium, 2.2mm Opening | \$ |
| 70020 | Source Holder for Cesium, 5mm Opening, for 90008 HDR 1000 Plus | \$ |
| 70009 | Source Holder for Low Dose Rate Iridium Ribbons | \$ |
| 70016 | Source Holder for Single LDR Seeds, 1.2mm Opening | \$ |
| 70022 | Source Holder for LDR Seed Batch Assay (up to 500 Pd or I Seeds & Iridium Wire Coil) | \$ |
| 70023 | Source Holder for RAPID Strand™ Iodine Seeds | \$ |
| 70024 | Source Holder for MICK Cartridge | \$ |
| 70026 | Source Holder for 5cc and 10cc Metastron™ Syringes & 153 Samarium | \$ |
| 70008 | Quality Assurance Tool Insert | \$ |
| 70110 | BEBIG Co-60 Afterloader Source Holder | \$ |

SOURCE HOLDERS FOR IVB 1000 CHAMBER AVAILABLE UPON REQUEST

Purchase Order Number:

- I authorize Standard Imaging to perform minor repairs or battery replacement, which may cost up to \$200
- I authorize Standard Imaging to perform service up to the following amount: \$ _____

Return shipping is UPS Blue unless otherwise requested.

| | |
|---|---|
| <p>Ship To</p> <p>Contact Name _____</p> <p>Location _____</p> <p>Address _____</p> <p>City, State, Zip _____</p> <p>Country _____</p> <p>Phone # or email _____</p> | <p>Bill To</p> <p>Contact Name _____</p> <p>Location _____</p> <p>Address _____</p> <p>City, State, Zip _____</p> <p>Country _____</p> <p>Phone # or email _____</p> |
|---|---|

If purchase order number included, this form represents a firm purchase order upon which to invoice for the selected items.
If any questions, please contact customer service at: support@standardimaging.com or call +1-608-831-0025 (International), 800-261-4446 (U.S.).